

This document contains information proprietary to Rosemount Analytical, and is not to be made available to those who may compete with Rosemount Analytical.

REVISION					
LTR	ECO	DESCRIPTION	BY	DATE	CHK

D 1400230

INFRARED REMOTE CONTROL UNIT (RMT PN 23572-00) FOR USE IN CLASS I AREA ONLY

MODEL 5081-G-FF XMTR



HAZARDOUS AREA
 IS CLASS I, GRPS A-D
 CLASS II, GRPS E-G
 CLASS III
 NI CLASS I, DIV 2
 GRPS A-D
 CLASS II, DIV 2
 GRPS E-G

UNCLASSIFIED AREA

ANY CSA APPROVED OR SIMPLE APPARATUS DEVICE

TB1-
 SHIELD 1
 BLK 7
 WHT 8
 RED 8
 GRY 10

5081-G CABLE SUPPLIED BY ROSEMOUNT ANALYTICAL ORRVILLE:
 1ST WIRE PAIR: #20 AWG
 2ND WIRE PAIR AND DRAIN: #22 AWG

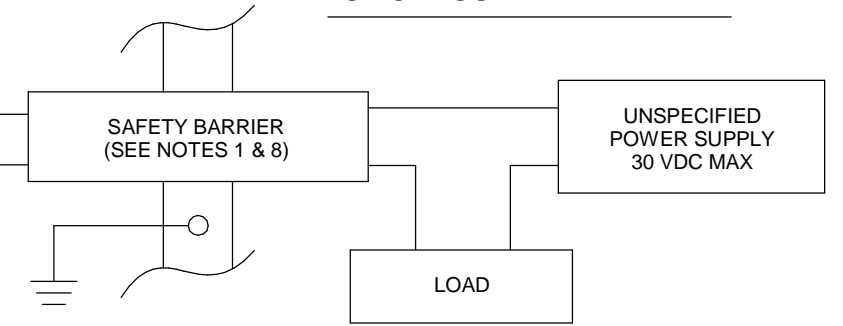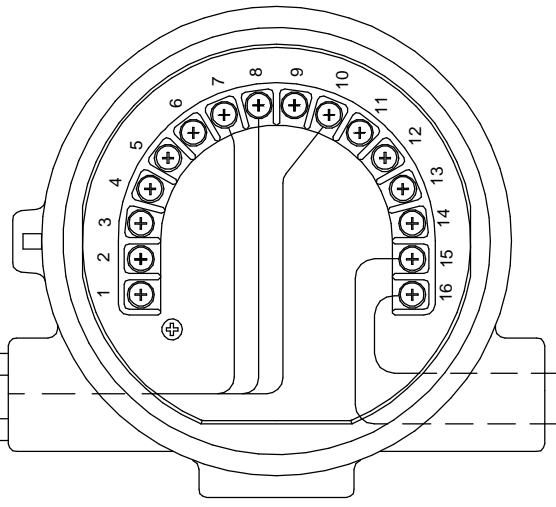

WARNING- SUBSTITUTION OF COMPONENTS MAY IMPAIR INTRINSIC SAFETY OR SUITABILITY FOR DIVISION 2.
WARNING- TO PREVENT IGNITION OF FLAMMABLE OR COMBUSTIBLE ATMOSPHERES, DISCONNECT POWER BEFORE SERVICING.

THIS DOCUMENT IS CERTIFIED BY
 CSA REV. A
 _____ REV. _____
 _____ REV. _____
 _____ REV. _____
 _____ REV. _____
 _____ REV. _____
 REVISIONS NOT PERMITTED W/O AGENCY APPROVAL

ITEM	PART NO.	DESCRIPTION	QTY
UNLESS OTHERWISE SPECIFIED TOLERANCES XX ± .030 ANGLES ± 1/2° .XXX ± .010 DIMENSIONS ARE IN INCHES REMOVE BURRS & SHARP EDGES .020 MAX MACHINED FILLET RADI .020 MAX NOMINAL SURFACE FINISH 125			
BILL OF MATERIAL			
APPROVALS		DATE	TITLE
DRAWN	N. KOUMBIS	07/14/03	Uniloc <small>Rosemount Analytical, Uniloc Division 2400 Berranca Pkwy Irvine, CA 92606</small>
CHECKED	D. CROWLEY	08/05/03	
PROJECT ENGR APVD	D. CROWLEY	08/05/03	
THIS DWG CONVERTED TO SOLID EDGE		D SIZE	REV A
02-06-04		9879	1400230
RELEASE DATE	ECO NO.	REV	SCALE NONE TYPE SHEET 1 OF 2

NOTES ON SHEET 2 OF 2
 NOTES: UNLESS OTHERWISE SPECIFIED

8 7 6 5 4 3 2 1

This document contains information proprietary to Rosemount Analytical, and is not to be made available to those who may compete with Rosemount Analytical.

- 12. NO REVISION TO DRAWING WITHOUT PRIOR CSA APPROVAL.
- 11. THE ASSOCIATED APPARATUS MUST BE CSA APPROVED.
- 10. CONTROL EQUIPMENT CONNECTED TO ASSOCIATED APPARATUS MUST NOT USE OR GENERATE MORE THAN 250 Vrms OR Vdc.
- 9. ASSOCIATED APPARATUS MANUFACTURER'S INSTALLATION DRAWING MUST BE FOLLOWED WHEN INSTALLING THIS EQUIPMENT.
- 8. THE ENTITY CONCEPT ALLOWS INTERCONNECTION OF INTRINSICALLY SAFE APPARATUS WITH ASSOCIATED APPARATUS WHEN THE FOLLOWING IS TRUE:

FIELD DEVICE INPUT	ASSOCIATED APPARATUS OUTPUT
Vmax OR Ui	Voc, Vt OR Uo;
Imax OR Ii	Isc, It OR Io;
Pmax OR Pi	Po;
Ci+ C cable;	Ca, Ct OR Co
Li+ L cable.	La, Lt OR Lo
- 7. RESISTANCE BETWEEN INTRINSICALLY SAFE GROUND AND EARTH GROUND MUST BE LESS THAN 1.0 Ohm.
- 6. DUST-TIGHT CONDUIT SEAL MUST BE USED WHEN INSTALLED IN CLASS II AND CLASS III ENVIRONMENTS.
- 5. SENSORS SHALL MEET THE REQUIREMENTS OF SIMPLE APPARATUS AS DEFINED IN ANSI/ISA RP12.06.01 AND THE CEC (CSA C22.1). THEY CAN NOT GENERATE NOR STORE MORE THAN 1.5V, 0.1A, 25mW OR A PASSIVE COMPONENT THAT DOES NOT DISSIPATE MORE THAN 1.3W. SEE TABLES I AND II.
- 4. INSTALLATION SHOULD BE IN ACCORDANCE WITH ANSI/ISA RP12.06.01 "INSTALLATION OF INTRINSICALLY SAFE SYSTEMS FOR HAZARDOUS (CLASSIFIED) LOCATIONS" AND THE CANADIAN ELECTRICAL CODE (CSA C22.1).
- 3. INTRINSICALLY SAFE APPARATUS (MODEL 5081-G-FF, FIELDBUS TERMINATOR AND ANY ADDITIONAL FIELDBUS DEVICES) AND ASSOCIATED APPARATUS (SAFETY BARRIER) SHALL MEET THE FOLLOWING REQUIREMENTS: THE VOLTAGE (Vmax) AND CURRENT (Imax) OF THE INTRINSICALLY SAFE APPARATUS MUST BE EQUAL TO OR GREATER THAN THE VOLTAGE (Voc OR Vt) AND CURRENT (Isc OR It) WHICH CAN BE DELIVERED BY THE ASSOCIATED APPARATUS (SAFETY BARRIER). IN ADDITION, THE MAXIMUM UNPROTECTED CAPACITANCE (Ci) AND INDUCTANCE (Li) OF THE INTRINSICALLY SAFE APPARATUS, INCLUDING INTERCONNECTING WIRING, MUST BE EQUAL OR LESS THAN THE CAPACITANCE (Ca) AND INDUCTANCE (La) WHICH CAN BE SAFELY CONNECTED TO THE APPARATUS. (REF. TABLES I, II & III).
- 2. THE CAPACITANCE AND INDUCTANCE OF THE LOAD CONNECTED TO THE SENSOR TERMINALS MUST NOT EXCEED THE VALUES SPECIFIED IN TABLE I
 WHERE $Ca \geq Ci$ (SENSOR) + C cable;
 $La \geq Li$ (SENSOR) + L cable.
- 1. ANY SINGLE SHUNT ZENER DIODE SAFETY BARRIER APPROVED BY CSA HAVING THE FOLLOWING OUTPUT PARAMETERS:
 SUPPLY/SIGNAL TERMINALS TB1-15, 16

 Voc OR Vt GREATER THAN 13 V BUT NOT GREATER THAN 30 V
 Isc OR It NOT GREATER THAN 300 mA
 Pmax NOT GREATER THAN 1.3 W

TABLE I

GAS GROUPS	OUTPUT PARAMETERS	
	Ca (uF)	La (mH)
A, B	10.63	4.28
C	488.63	17.9
D	10,000	34.9

TABLE II

OUTPUT PARAMETERS	MODEL 5081-G-FF TB1-1 THRU 12
Vt	6.51 V
It	86.8 mA
Pt	141.27 mA

TABLE III

5081-G-FF ENTITY PARAMETERS SUPPLY / SIGNAL TERMINALS TB 1-15, 16					
MODEL NO.	Vmax (Vdc)	Imax (mA)	Pmax (W)	Ci (pF)	Li (mH)
5081-G-FF	30	300	1.3	564	0

NOTES: UNLESS OTHERWISE SPECIFIED

D	DWG NO. 1400230	REV A
SCALE: NONE	TYPE	SHEET 2 OF 2